



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM
DATAMASTER MAINTENANCE REPORT

RECEIVED

By Carol Day at 8:17 am, Oct 17, 2013 PORT #6

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 204081	NAME OF AGENCY MSHP	DATE OF INSPECTION 10/15/2013
LOCATION OF INSTRUMENT (STREET AND CITY) Scott County Sheriff's Office-S. New Madrid St.-Benton		TIME OF INSPECTION 9:36 am

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 10/15/2013 09:38
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER 50.0 °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER
<input checked="" type="checkbox"/> INDICATOR LIGHTS	
<input checked="" type="checkbox"/> SIMULATOR SOLUTION SUPPLIER Repco LOT # 13001 EXP. DATE 03/07/2015	
<input checked="" type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) 34.0 °C SIMULATOR SN 1099 EXP. DATE 02/20/2014	
<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)	
Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)	
<input checked="" type="checkbox"/> 0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE	
<input type="checkbox"/> 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE	
<input type="checkbox"/> 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE	
TEST 1 * .098	TEST 2 * .099
TEST 3 * .100	

☒ PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:
(DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	0	(0-.04)	0	(.05-.09)	1	(.10-.14)	0	(.15-.19)	0	OVER .19	0
----------	---	---------	---	-----------	---	-----------	---	-----------	---	----------	---

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS
(USE OTHER SIDE IF NECESSARY).

INSPECTING OFFICER

SIGNATURE <i>James C. Cooksey Jr.</i>	PRINT FULL NAME James C. Cooksey Jr.
TYPE II PERMIT NUMBER/EXPIRATION DATE 230016 02/08/2015	TELEPHONE NUMBER (573) 840-9500

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office
2875 James Blvd.
Poplar Bluff, MO 63901

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.
LOT NUMBER: 13001
EXPIRATION DATE: March 7, 2015 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:


RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 13001 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1215 gms/dl \pm .003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 \pm 3% gms/210L Breath when heated to 34 Degrees Celsius \pm 0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is March 8, 2013
The expiration date for this lot number is March 7, 2015 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President
RepCo Marketing, Inc.

Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

MISSOURI STATE HIGHWAY PATROL
BAC DATAMASTER SERIAL NUMBER 204081
10/15/13
89138


--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM (04-67-2009):	OKAY
HEATERS	
SAMPLE CHAMBER:	50c
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!"#\$%&'()*+,-./:;<=123456789*!<=>?@AB CDEFG
HIJKLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~>?"

Operator Signature



Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

MISSOURI STATE HIGHWAY PATROL
BAC DATAMASTER SERIAL NUMBER 204001
10/13/13

ARREST TIME: 09:20

SUBJECT NAME:

TEST

DOB: 01/01/96 SEX: M

STATE/D.L.: MO/129856

ARRESTING OFFICER:

COOKSEY/JAMES/C

OFFICER I.D.: 266

TESTING OFFICER:

COOKSEY/JAMES/C

OFFICER I.D.: 266

PERMIT NUMBER: 200016

EXPIRATION DATE: 02/08/15


MISCELLANEOUS DATA:

RFI TEST

--- BREATH ANALYSIS ---

RADIO INTERFERENCE

Operator Signature

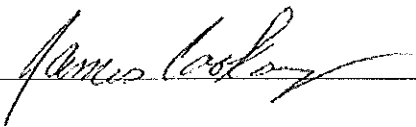

Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

MISSOURI STATE HIGHWAY PATROL
BAC DATAMASTER SERIAL NUMBER 204001
10/15/13

TESTING OFFICER:

COOKSEY/JAMES/C

OFFICER I.D.: 266

PERMIT NUMBER: 200016

EXPIRATION DATE: 02/08/15

MISCELLANEOUS DATA:

MAINTENANCE

--- SUPERVISOR MODE ---


BLANK TEST	.000	09:50
INTERNAL STANDARD	VERIFIED	09:51
EXTERNAL STANDARD	.098	09:51
BLANK TEST	.000	09:52
EXTERNAL STANDARD	.099	09:52
BLANK TEST	.000	09:53
EXTERNAL STANDARD	.100	09:53
BLANK TEST	.000	09:54

N = 3

SIM. = .1

AVG. = .099

Operator Signature

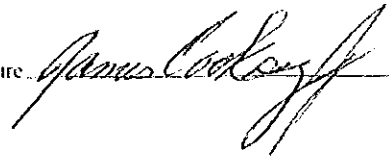



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM



PERMIT
TYPE II

JAMES C COOKSEY JR

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 02/08/2013

NUMBER 230016

EXPIRES 02/08/2015

MO 580-0771 (8-10)

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

W. W. Cooksey Jr.
W. W. Cooksey Jr.

Acting Director

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LAB-4 (RS-10)